



Alkaline Phosphatase Microplate Assay Kit

Catalog # AS0003

Detection and Quantification of Alkaline Phosphatase Activity in
Urine, Serum, Plasma, Tissue extracts, Cell lysate, Cell culture media
and Other biological fluids Samples.

This instruction must be read in its entirety before using this product.

For research use only, Not for use in diagnostic procedures.

Contact information:

Tel:+1 (301) 446-2499 Fax:+1 (301) 446-2413

Email:techcn@signalwayantibody.com Web:www.sabbiotech.com

I. INTRODUCTION.....	2
II. KIT COMPONENTS.....	3
III. MATERIALS REQUIRED BUT NOT PROVIDED.....	3
VI. SAMPLE PREPARATION.....	4
V. ASSAY PROCEDURE.....	5
VI. CALCULATION.....	6
VII. TYPICAL DATA.....	7
VIII. TECHNICAL SUPPORT.....	7
IX. NOTES.....	7

I. INTRODUCTION

Alkaline phosphatase (ALP) catalyzes the hydrolysis of phosphate esters in an alkaline environment, resulting in the formation of an organic radical and inorganic phosphate. In mammals, this enzyme is found mainly in the liver and bones. Marked increase in serum ALP levels, a disease known as hyperalkalinephosphatasemia, has been associated with malignant biliary obstruction, primary biliary cirrhosis, primary sclerosing cholangitis, hepatic lymphoma and sarcoidosis.

The assay is initiated with the enzymatic hydrolysis of the disodium phenyl phosphate by alkalinephosphatase. The enzyme catalysed reaction products can be measured at a colorimetric readout at 510 nm.

II. KIT COMPONENTS

Component	Volume	Storage
96-Well Microplate	1 plate	
Assay Buffer	30 ml x 4	4 °C
Reaction Buffer	4 ml x 1	4 °C, keep in dark
Substrate	Powder x 1	4 °C, keep in dark
Dye Reagent I	Powder x 1	4 °C, keep in dark
Dye Reagent II	Powder x 1	4 °C, keep in dark
Standard	Powder x 1	4 °C
Plate Adhesive Strips	3 Strips	
Technical Manual	1 Manual	

Note:

Substrate: add 4 ml distilled water to dissolve before use.

Dye Reagent I: add 10 ml distilled water to dissolve before use.

Dye Reagent II: add 2 ml distilled water to dissolve before use.

Standard: add 1 ml distilled water to dissolve, then add 40 µl standard into 960 µl distilled water, the concentration will be 4mmol/L.

III. MATERIALS REQUIRED BUT NOT PROVIDED

1. Microplate reader to read absorbance at 510 nm
2. Distilled water
3. Pipettor
4. Pipette tips
5. Mortar
6. Ice
7. Centrifuge
8. Timer

IV. SAMPLE PREPARATION

1. For cell and bacteria samples

Collect cell or bacteria into centrifuge tube, discard the supernatant after centrifugation, add 1 ml Assay buffer for 5×10^6 cell or bacteria, sonicate (with power 20%, sonication 3s, interval 10s, repeat 30 times); centrifuged at 8000g 4°C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

2. For tissue samples

Weigh out 0.1 g tissue, homogenize with 1 ml Assay buffer on ice, centrifuged at 8000g 4°C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

3. For serum or plasma samples

Detect directly, or dilute with Assay Buffer.

V. ASSAY PROCEDURE

Add following reagents in the microplate:

Reagent	Sample	Standard	Blank
Sample	10µl	--	--
Standard	--	10µl	--
Distilled water	--	--	10µl
Reaction Buffer	40 µl	40 µl	40 µl
Substrate	40 µl	40 µl	40 µl
Mix, put it in the oven,37 °C for 15 minutes.			
Dye Reagent I	100 µl	100 µl	100 µl
Dye Reagent II	20 µl	20 µl	20 µl
Mix,wait for 10 minutes, record absorbance measured at 510 nm.			

VI. CALCULATION

Unit Definition: One unit of Alkaline Phosphatase activity is defined as the enzyme generates 1 nmolphenol per minute.

1. According to the protein concentration of sample

$$\begin{aligned} \text{ALP (U/mg)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / V_{\text{Sample}} / \\ & C_{\text{Protein}} / T \\ &= 266.67 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / C_{\text{Protein}} \end{aligned}$$

2. According to the weight of sample

$$\begin{aligned} \text{ALP (U/g)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (V_{\text{Sample}} \times W / \\ & V_{\text{Assay}}) / T \\ &= 266.67 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / W \end{aligned}$$

3. According to the volume of serum or plasma

$$\begin{aligned} \text{ALP (U/ml)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / V_{\text{Sample}} / T \\ &= 266.67 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) \end{aligned}$$

C_{Protein} : the protein concentration of sample, mg/ml;

W : the weight of sample, g;

C_{Standard} : the concentration of standard, 4mmol/L = 4000 nmol/ml;

V_{Standard} : the volume of standard, 0.01 ml;


V_{Sample} : the volume of sample, 0.01 ml;

V_{Assay} : the volume of Assay buffer, 1 ml;

T : the reaction time, 15 minutes.

VII. TYPICAL DATA

The standard curve is for demonstration only. A standard curve must be run with each assay.

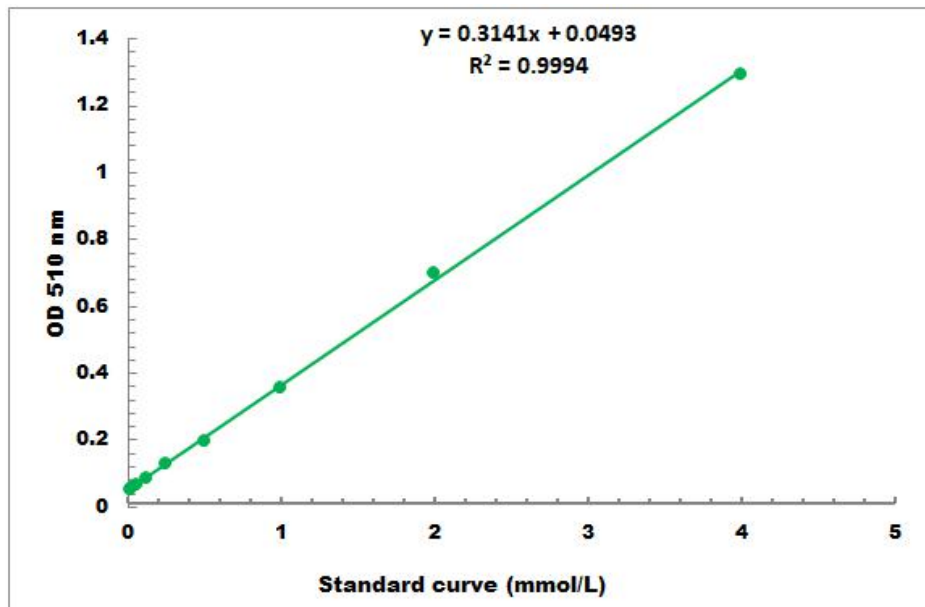

Detection Range: 0.04mmol/L -4mmol/L

VIII. TECHNICAL SUPPORT

For troubleshooting, information or assistance, please go online to www.sabbitech.cn or contact us at techcn@signalwayantibody.com

IX. NOTES