



Neutral Xylanase Microplate Assay Kit

Catalog # AS0089

Detection and Quantification of Neutral Xylanase Activity in Animal feeds, Enzyme preparations, Bread improver mixtures and other materials Samples.

This instruction must be read in its entirety before using this product.

For research use only, Not for use in diagnostic procedures.

Contact information:

Tel:+1 (301) 446-2499 Fax:+1 (301) 446-2413

Email:techcn@signalwayantibody.com Web:www.sabbiotech.com

I. INTRODUCTION.....	2
II. KIT COMPONENTS.....	3
III. MATERIALS REQUIRED BUT NOT PROVIDED.....	3
VI. SAMPLE PREPARATION.....	4
V. ASSAY PROCEDURE.....	5
VI. CALCULATION.....	6
VII. TYPICAL DATA.....	7
VIII. TECHNICAL SUPPORT.....	7
IX. NOTES.....	7

I. INTRODUCTION

Xylanase (EC 3.2.1.8) is the name given to a class of enzymes which degrade the linear polysaccharide beta-1,4-xylan into xylose, thus breaking down hemicellulose, one of the major components of plant cell walls. As such, it plays a major role in micro-organisms thriving on plant sources for the degradation of plant matter into usable nutrients. Xylanases are produced by fungi, bacteria, yeast, marine algae, protozoans, snails, crustaceans, insect, seeds, etc., (mammals do not produce xylanases).

The assay is initiated with the enzymatic hydrolysis of the xylan by neutral xylanase. The enzyme catalysed reaction products react with 3,5-dinitrosalicylic acid, and can be measured at a colorimetric readout at 540 nm.

II. KIT COMPONENTS

Component	Volume	Storage
96-Well Microplate	1 plate	
Assay Buffer	30 ml x 4	4 °C
Substrate	Powder x 1	4 °C
Dye Reagent	10 ml x 1	4 °C, keep in dark
Standard(2.5µmol/ml)	1 ml x 1	4 °C
Plate Adhesive Strips	3 Strips	
Technical Manual	1 Manual	

Note:

Substrate: add 10 ml Assay Buffer to dissolve before use, store at 4 °C.

III. MATERIALS REQUIRED BUT NOT PROVIDED

1. Microplate reader to read absorbance at 540 nm
2. Distilled water
3. Pipettor
4. Pipette tips
5. Mortar
6. Centrifuge
7. Timer
8. Convection oven

IV. SAMPLE PREPARATION

1. For animal feeds, enzyme preparations, bread improver mixtures samples

Weigh out 0.1 g sample, homogenize with 1 ml Assay buffer, centrifuged at 8,000g 4°C for 20 minutes, take the supernatant into a new centrifuge tube for detection.

2. For liquid sample

Add 0.1 ml sample into 0.9 ml Assay buffer, Centrifuged at 8,000g 4°C for 20 minutes, take the supernatant into a new centrifuge tube for detection.

V. ASSAY PROCEDURE

Add following reagents in the microcentrifuge tube:

Reagent	Sample	Control	Standard	Blank
Sample	10 μ l	--	--	--
Distilled water	--	10 μ l	--	--
Substrate	90 μ l	90 μ l	--	--
Mix, put it in the oven, 50°C for 10 minutes.				
Standard	--	--	100 μ l	--
Distilled water	--	--	--	100 μ l
Dye Reagent	100 μ l	100 μ l	100 μ l	100 μ l
Mix, put it into the convection oven, 90°C for 10 minutes, when cold record absorbance measured at 540 nm.				

VI. CALCULATION

Unit Definition: One unit of Neutral Xylanase activity is the enzyme that generates 1 μmol of reducing sugar per hour at 50°C, pH6.0.

1. According to the weight of sample

$$\begin{aligned} \text{NEX (U/g)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (V_{\text{Sample}} \times W / \\ &\quad V_{\text{Assay}}) / T \\ &= 2.5 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / W \end{aligned}$$

2. According to the volume of sample

$$\begin{aligned} \text{NEX (U/ml)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (V_{\text{Sample}} \times V \\ &\quad / V_{\text{Assay}}) / T \\ &= 2.5 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / V \end{aligned}$$

C_{Standard} : the concentration of Standard, 2.5 μmol/ml;

W : the weight of sample, g;

V : the volume of sample, ml;

V_{Standard} : the volume of standard, 0.1 ml;


V_{Sample} : the volume of sample, 0.01 ml;

V_{Assay} : the volume of Assay buffer in sample preparation, 1 ml;

T : the reaction time, 10 minutes.

VII. TYPICAL DATA

The standard curve is for demonstration only. A standard curve must be run with each assay.

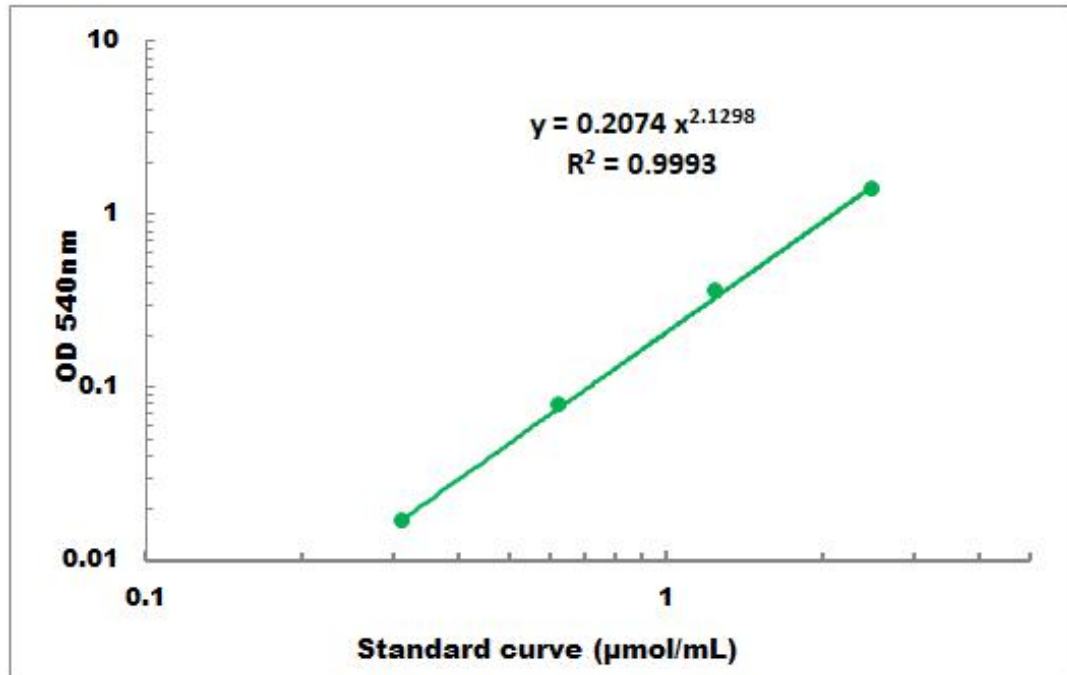

Detection Range: 0.25µmol/mL - 2.5µmol/mL

VIII. TECHNICAL SUPPORT

For troubleshooting, information or assistance, please go online to www.sabbiotech.cn or contact us at techcn@signalwayantibody.com

IX. NOTES