



Glucose Dehydrogenase Microplate Assay Kit

Catalog # AS0182

Detection and Quantification of Glucose Dehydrogenase Activity in Serum, Plasma, Tissue extracts, Cell lysate, Cell culture media, Other biological fluids Samples.

This instruction must be read in its entirety before using this product.

For research use only, Not for use in diagnostic procedures.

Contact information:

Tel:+1 (301) 446-2499 Fax:+1 (301) 446-2413

Email:techcn@signalwayantibody.com Web:www.sabbiotech.com

I. INTRODUCTION.....	2
II. KIT COMPONENTS.....	3
III. MATERIALS REQUIRED BUT NOT PROVIDED.....	3
VI.SAMPLE PREPARATION.....	4
V. ASSAY PROCEDURE.....	5
VI. CALCULATION.....	6
VII. TECHNICAL SUPPORT.....	7
VIII. NOTES.....	7

I. INTRODUCTION

Glucose Dehydrogenase (GDH) (EC 1.1.1.118) is an enzyme that catalyzes the chemical reaction: $D\text{-glucose} + \text{NAD}^+ \leftrightarrow D\text{-glucono-1,5-lactone} + \text{NADH} + \text{H}^+$. This enzyme belongs to the family of oxidoreductases, specifically those acting on the CH-OH group of donor with NAD^+ or NADP^+ as acceptor.

Glucose Dehydrogenase Microplate Assay Kit provides a convenient tool for sensitive detection of the GDH in a variety of samples. The GDH present in sample will recognize D-glucose as a specific substrate leading to a proportional color development. The activity is determined by measuring the increase in absorbance at 340 nm resulting from NADH.

II. KIT COMPONENTS

Component	Volume	Storage
96-Well Microplate	1 plate	
Assay Buffer	30 ml x 4	4 °C
Substrate	Powder x 1	-20 °C
Reaction Buffer	10 ml x 1	4 °C
Standard	Powder x 1	-20 °C
Positive Control	Powder x 1	-20 °C
Technical Manual	1 Manual	

Note:

Substrate: add 2 ml Assay Buffer to dissolve before use.

Standard: add 1 ml distilled water to dissolve before use; then add 0.2 ml into 0.8 ml distilled water, the concentration will be 400 $\mu\text{mol/L}$.

Positive Control: add 1 ml Assay Buffer to dissolve before use.

III. MATERIALS REQUIRED BUT NOT PROVIDED

1. Microplate reader to read absorbance at 340 nm
2. Distilled water
3. Pipettor
4. Pipette tips
5. Mortar
6. Centrifuge
7. Timer
8. Ice

IV. SAMPLE PREPARATION

1. For cell and bacteria samples

Collect cell or bacteria into centrifuge tube, discard the supernatant after centrifugation, add 1 ml Assay buffer for 5×10^6 cell or bacteria, sonicate (with power 20%, sonication 3s, interval 10s, repeat 30 times); centrifuged at 8000g 4°C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

2. For tissue samples

Weigh out 0.1 g tissue, homogenize with 1 ml Assay buffer on ice, centrifuged at 8000g 4°C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

3. For liquid samples

Detect directly, or dilute with Assay Buffer.

V. ASSAY PROCEDURE

Warm all reagents to room temperature before use.

Add following reagents into the microplate:

Reagent	Sample	Control	Standard	Blank	Positive Control
Standard	--	--	200 μ l	--	--
Distilled water	--	10 μ l	--	200 μ l	--
Substrate	100 μ l	100 μ l	--	--	100 μ l
Reaction Buffer	90 μ l	90 μ l	--	--	90 μ l
Sample	10 μ l	--	--	--	--
Positive Control	--	--	--	--	10 μ l

Mix, incubate at measured at 37 °C for 5 min, record the absorbance at 340 nm.

Note: if the enzyme activity is lower, please add more sample into the reaction system; or increase the reaction time.

VI. CALCULATION

Unit Definition: One unit of GDH activity is defined as the enzyme produce 1nmolNADH per minute.

1. According to the protein concentration of sample

$$\text{GDH (U/mg)} = \frac{(C_{\text{Standard}} \times V_{\text{Standard}}) \times (OD_{\text{Sample}} - OD_{\text{Control}}) / (OD_{\text{Standard}} - OD_{\text{Blank}})}{(V_{\text{Sample}} \times C_{\text{Protein}}) / T}$$

$$= 1600 \times (OD_{\text{Sample}} - OD_{\text{Control}}) / (OD_{\text{Standard}} - OD_{\text{Blank}}) / C_{\text{Protein}}$$

2. According to the weight of sample

$$\text{GDH (U/g)} = \frac{(C_{\text{Standard}} \times V_{\text{Standard}}) \times (OD_{\text{Sample}} - OD_{\text{Control}}) / (OD_{\text{Standard}} - OD_{\text{Blank}})}{(V_{\text{Sample}} \times W / V_{\text{Assay}}) / T}$$

$$= 1600 \times (OD_{\text{Sample}} - OD_{\text{Control}}) / (OD_{\text{Standard}} - OD_{\text{Blank}}) / W$$

3. According to the quantity of cells or bacteria

$$\text{GDH (U/10}^4\text{)} = \frac{(C_{\text{Standard}} \times V_{\text{Standard}}) \times (OD_{\text{Sample}} - OD_{\text{Control}}) / (OD_{\text{Standard}} - OD_{\text{Blank}})}{(V_{\text{Sample}} \times N / V_{\text{Assay}}) / T}$$

$$= 1600 \times (OD_{\text{Sample}} - OD_{\text{Control}}) / (OD_{\text{Standard}} - OD_{\text{Blank}}) / N$$

4. According to the volume of sample

$$\text{GDH (U/ml)} = \frac{(C_{\text{Standard}} \times V_{\text{Standard}}) \times (OD_{\text{Sample}} - OD_{\text{Control}}) / (OD_{\text{Standard}} - OD_{\text{Blank}})}{V_{\text{Sample}} / T}$$

$$= 1600 \times (OD_{\text{Sample}} - OD_{\text{Control}}) / (OD_{\text{Standard}} - OD_{\text{Blank}})$$

C_{Standard} : the standard concentration, 400 $\mu\text{mol/L}$ = 400nmol/ml;

V_{Standard} : the volume of standard, 200 μl = 0.2 ml;

C_{Protein} : the protein concentration, mg/ml;

W: the weight of sample, g;

N: the quantity of cell or bacteria, $N \times 10^4$;


V_{Sample} : the volume of sample, 0.01 ml;

V_{Assay} : the volume of Assay buffer, 1 ml;


T: the reaction time, 5 minutes.

VII. TYPICAL DATA

The standard curve is for demonstration only. A standard curve must be run with each assay.

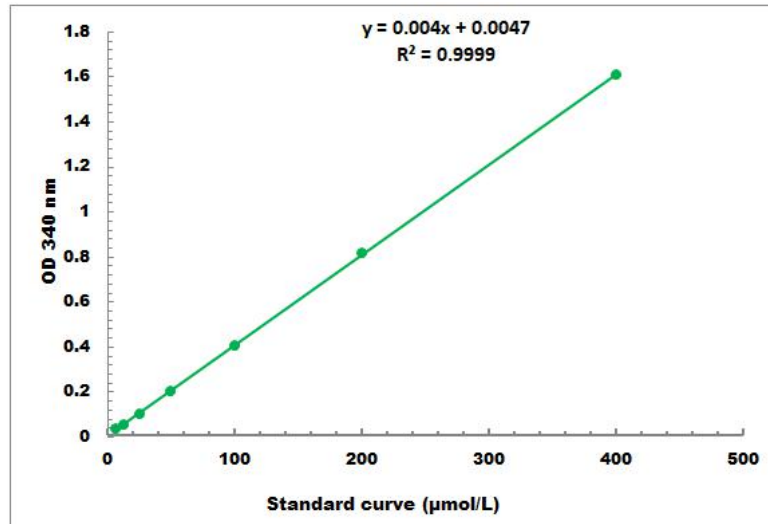

Detection Range: 4µmol/L - 400 µmol/L

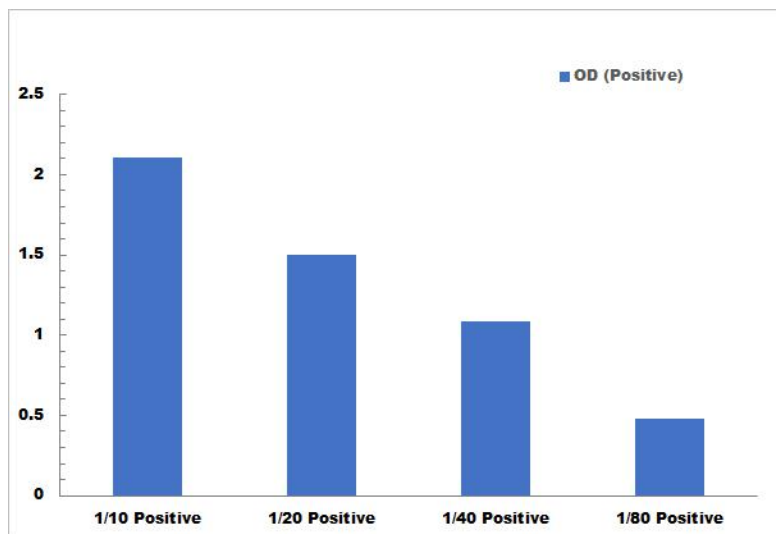

Positive Control reaction in 96-well plate assay with decreasing the concentration

VIII. TECHNICAL SUPPORT

For troubleshooting, information or assistance, please go online to www.sabbiotech.cn or contact us at techcn@signalwayantibody.com

IX. NOTES